



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification<sup>6</sup> : <b>A61B 17/00</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 96/18343</b> (43) International Publication Date: 20 June 1996 (20.06.96)</p>
<p>(21) International Application Number: PCT/US95/16022 (22) International Filing Date: 12 December 1995 (12.12.95) (30) Priority Data: 08/355,142 13 December 1994 (13.12.94) US (60) Parent Application or Grant (63) Related by Continuation US 08/355,142 (CIP) Filed on 13 December 1994 (13.12.94) (71) Applicant (for all designated States except US): MICRO INTERVENTIONAL SYSTEMS, INC. [US/US]; Suite 2, 680 West Maude Avenue, Sunnyvale, CA 94086 (US). (72) Inventors; and (75) Inventors/Applicants (for US only): MCGURK, Erin [US/US]; 323 Stanford Avenue, Palo Alto, CA 94306 (US). DIECK, Ronald [US/US]; 323 Stanford Avenue, Palo Alto, CA 94306 (US). TREMULIS, William, S. [US/US]; 97 Pelican Lane, Redwood City, CA 94065 (US).</p>		<p>(74) Agents: HESLIN, James, M. et al.; Townsend and Townsend and Crew, Steuart Street Tower, 20th floor, One Market Plaza, San Francisco, CA 94105 (US). (81) Designated States: CA, JP, US, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  Published <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>
<p>(54) Title: EMBOLIC ELEMENTS AND METHODS AND APPARATUS FOR THEIR DELIVERY</p> <div data-bbox="308 1108 1315 1491"> </div> <p>(57) Abstract</p> <p>An embolic element (10) comprises a filament composed of a shape memory material having an unexpanded coil configuration and an expanded random matrix configuration. The embolic element (10) may be delivered to a blood vessel (BV) treatment site in its coiled configuration over a delivery wire (30) through a guide catheter (44). Usually, the coiled embolic element (10) will be disposed over a helical section of the delivery wire (30) prior to release. In that way, proper positioning of the embolic element (10) is then expanded to its enlarged configuration by heating or otherwise exposing to a temperature over the transition temperature of the shape memory material.</p>		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
BJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

## EMBOLIC ELEMENTS AND METHODS AND APPARATUS FOR THEIR DELIVERY

This application is a continuation-in-part of application serial no. 08/355,142, filed on December 13, 1994, the full disclosure of which is incorporated herein by reference.

5

### BACKGROUND OF THE INVENTION

#### 1. Field of the Invention

The present invention relates generally to the field of medical devices and procedures and more particularly to the structure and deployment of embolic elements for occluding target sites, such as aneurysms, within a blood vessel.

Embolic coils, also referred to as vaso-occlusion coils, are used for selectively occluding blood vessels for a variety of purposes, such as the control of internal bleeding, the occlusion of blood supply to tumors, and the blocking of blood flow to aneurysms. Of particular interest to the present invention, embolic coils may be delivered to brain aneurysms by first positioning the distal end of a small tubular catheter through an opening in the blood vessel wall to the aneurysm and then pushing a plurality of embolic coils into the aneurysm volume. The coils then occlude the aneurysm by promoting thrombus formation.

While being generally successful, such treatment methods suffer from certain deficiencies. Most embolic coils display little or no expansion when they are released from their delivery catheters. One type of coil, which achieves perhaps the best expansion ratio, is delivered through the catheter as a straightened wire filament. Upon release from the catheter, the wire assumes a preset coil configuration within the aneurysm. The resulting coil, however, does not maximize the volume occupied by the embolic device. A second common approach relies on pushing an embolic coil through a

delivery catheter with the coil in its coiled configuration. As the embolic coil is released, it further deploys with a secondary helical configuration, increasing the effective width of the coil, but decreasing its length. Again, the  
5 resulting occluded volume has not been maximized.

Conventional embolic coil delivery techniques also suffer from a lack of control. In many cases, the embolic coils are pushed through the distal end of the delivery catheter and released without any control over their  
10 positioning. While certain improvements have been proposed, such as where the embolic coil is attached to a pusher wire and released from the wire only after some positioning of the coil within the aneurysm, the control over positioning is quite limited.

15 It would therefore be desirable to provide improved embolic element structures and methods and apparatus for their delivery and deployment. In particular, it would be desirable to provide embolic element structures which possess both a compact delivery configuration and a maximally expanded  
20 released configuration in order to increase the occlusive volume of the element. It would be further desirable to provide embolic element delivery systems and methods which can control placement and positioning of the embolic element within a blood vessel target site, such as an aneurysm, prior  
25 to release of the embolic element into the site. It would be particularly desirable if the embolic element could be deployed in a preselected three-dimensional configuration prior to release into the site.

30 2. Description of the Background Art

Embolic coils and catheter delivery systems for such coils are described in U.S. Patent Nos. 4,994,069; 5,108,407; 5,122,136; 5,217,484; 5,226,911; 5,234,437; 5,250,071; 5,261,916; and 5,312,415; and PCT applications WO 93/06503;  
35 WO 93/06884; WO 94/09705; WO 94/10936; and WO 94/11051. Endovascular placement of vascular appliances composed of shape memory materials is described in U.S. Patent Nos. 3,868,956; 4,170,990; 4,503,569; 4,512,338; 4,950,258;

and 5,067,957. The '956 patent described the *in situ* heating of vascular stents and filters to expand and anchor the devices within a blood vessel. Micro catheters and guidewires are described in U.S. Patent Nos. 4,739,768; 4,813,934; 5 4,884,579; and 5,109,867.

#### SUMMARY OF THE INVENTION

The present invention provides improved embolic elements and systems and methods for their delivery and deployment within a blood vessel for selective occlusion of a target site. The embolic elements have a very compact unexpanded configuration for delivery through or over a catheter and can be expanded to a much larger size to maximize the resulting occlusion volume. The delivery system and method permit pre-positioning of the embolic element within a predefined volume prior to release of the element into the target site.

According to the present invention, the embolic element comprises a filament composed of a shape memory material, where the filament is disposed in an unexpanded configuration at a first temperature at or below a transition temperature and assumes an expanded configuration when the temperature is raised to or above the transition temperature. Preferably, the unexpanded configuration will be a tightly-wound coil which minimizes the size of the embolic element for delivery through a catheter, as described in more detail below. The expanded configuration is preferably a random matrix where the filament uncoils to define a peripheral envelope which is larger in all dimensions than that of the coil or other unexpanded configuration. In particular, the peripheral envelope will have no transverse dimension which is less than the maximum dimension of the unexpanded embolic element, typically the length of the coil prior to expansion.

According to another aspect of the present invention, a system for selectively occluding a target location within a blood vessel comprises a catheter and an embolic element as described above. The catheter includes means for heating the embolic element to or above the

transition temperature when the element is positioned at the target location. The heating means may be electric, radiative, or fluid, with the preferred heating means comprising a lumen in the catheter for directing a heated  
5 medium past the embolic coil when positioned at the target location.

In a preferred aspect of the present invention, the delivery catheter has a tubular body with an axial lumen which receives the embolic element in its unexpanded configuration.  
10 The system further comprises a delivery wire having a helical section at its distal end. The embolic element, typically in its unexpanded coiled configuration, may be delivered over the delivery wire through the axial lumen of the delivery catheter. The helical section at the distal end of delivery  
15 catheter may be disposed within the target location, typically inside an aneurysm, so that the embolic element assumes the helical configuration prior to expansion and release from the catheter. In this way, positioning of the embolic element prior to release can be controlled. Additionally, by properly  
20 selecting the dimensions of the helical portion of the delivery wire, the expanded volume of the embolic element can be maximized.

In another preferred aspect of the present invention, the delivery wire of the delivery catheter  
25 comprises a selectively deployable gate at its distal end. The gate is intended to block premature or other unintended release of the embolic element from the delivery wire. The gate can be selectively "opened" when delivery is intended. Usually, the gate will be deployable between an expanded  
30 configuration that blocks passage of an embolic coil over the distal end of the wire in a non-expanded configuration which permits such passage. In an exemplary embodiment, the deployable gate is composed of a shape memory alloy which is formed into an expanded configuration which is retained at  
35 body temperature and which assumes its non-expanded configuration when exposed to an environment heated above body temperature, typically by exposure to heated saline from the catheter. In the specifically illustrated embodiment, the

gate is a slotted tube formed from, e.g., Nitinol, where the slotted region is deformed into an expanded malecott-type structure and which assumes its narrow-diameter, straightened configuration when forced back into the austenitic phase by exposure to heated saline above body temperature.

According to a first method of the present invention, an embolic element is delivered to a target site within a blood vessel by first positioning a delivery wire through a guide catheter so that a distal end of the delivery wire is disposed at the target site. The embolic element is then introduced over the delivery wire to the target site in an unexpanded configuration. The embolic element is expanded and released from the delivery wire at the target site by heating to a temperature above the transition temperature of the shape memory alloy. Such heating can be effected either by raising the temperature of the embolic element over body temperature (where the transition temperature exceeds body temperature) or by initially cooling the element below body temperature (where body temperature is at or above the transition temperature). Preferably, the delivery wire has a helix formed at its distal end so that the embolic element will assume a helical configuration prior to expansion and release at the target site.

According to a second method of the present invention, a target location in a blood vessel is occluded by introducing an embolic element composed of a shape memory alloy at the target location. The embolic element is heated above a transition temperature to cause expansion, and the target location is occluded by thrombus formation within the expanded volume of the embolic element. The target location is preferably an aneurysm and the embolic element is preferably delivered by the first method described above.

Optionally, the method of the present invention may comprise a further step of selectively permitting release of the embolic element from the delivery wire. In this way, retention of the embolic element on the catheter can be assured until such time as the intentional release is desired. In the specific embodiment, the selective release step comprises

exposing a heat memory alloy gate which blocks release of the coil to a temperature above body temperature, wherein the gate reconfigures from an expanded configuration which blocks passage of the element to a non-expanded configuration which permits passage of the element. Conveniently, the selective release may be effected by the infusion of a heated saline, typically in the same step which effects reconfiguration of the embolic coil as described above.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is a perspective view of an embolic element constructed in accordance with the principles of the present invention, shown in its unexpanded configuration in partial cross-section.

Fig. 2 is a perspective view of the embolic element of Fig. 1 shown in its expanded configuration.

Fig. 3 is an elevational view of a guide catheter used for introducing the embolic element of Fig. 1, shown in partial cross-section.

Fig. 4 is a perspective view of a delivery wire which may be used in combination with the guide catheter of Fig. 3 for introducing the embolic element of Fig. 1 according to the method of the present invention.

Fig. 5 is a coil pusher which may be used to advance the embolic element over the delivery wire of Fig. 4.

Figs. 6-11 illustrate use of a delivery system comprising the guide catheter, delivery wire, and coil pusher for introducing the embolic element of Fig. 1 to a target site within a blood vessel.

Figs. 12-14 illustrate the construction and use of a selective delivery gate on the delivery catheter of the present invention.

#### DESCRIPTION OF THE PREFERRED EMBODIMENT

The embolic element of the present invention is composed of a shape memory material, usually a shape memory metal alloy such as nickel-titanium alloy, available under the tradename Nitinol. Alternatively, the embolic elements may



be composed of shape memory plastics, such as homo- or co-polymers of lactide and/or glycolide, as described in U.S. Patent No. 4,950,258, the full disclosure of which is incorporated herein by reference. The embolic element will have an unexpanded configuration below a transition temperature (which is characteristic of the particular shape memory material utilized) and an expanded configuration which is attained when the element is exposed to a temperature at or above the transition temperature. The element may be delivered to the target site within a blood vessel in its unexpanded (compact) configuration and thereafter transformed to its expanded configuration in order to increase the occlusive volume provided by the element after release at the target site. The embolic element will be delivered to the target site at a temperature below the transition temperature, (typically being body temperature but optionally being a temperature below body temperature) and will be selectively transformed to the expanded configuration after release at the target site by exposure to a temperature at or above the transition temperature. Usually, the temperature change will be effected by heating the embolic element above body temperature, as will be the case when the element is delivered to the target site at body temperature. Alternatively, body temperature may be sufficient to effect expansion when the element is delivered to the target site at a temperature below body temperature.

In a preferred aspect of the present invention, the embolic element is a filament composed of a metal or plastic (polymeric) shape memory material having a diameter in the range from 0.01 mm to 0.1 mm, preferably from 0.02 mm to 0.05 mm, and a length in the range from about 30 cm to 1000 cm, preferably from 90 cm to 300 cm. In the unexpanded configuration of the embolic element, the filament is formed into a tightly-wound coil, typically having a diameter in the range from 0.1 mm to 1 mm, preferably from 0.25 mm to 0.5 mm, and a length in the range from 2 mm to 60 cm, preferably from 25 mm to 15 cm. The coil will usually have from 20 turns to 60,000 turns, usually from 1000 turns to 6000 turns. In th

expanded configuration of the embolic element, the filament opens into a random matrix or structure having a peripheral envelope which is larger in all dimensions than the maximum dimension of the initial coiled configuration. Usually, the peripheral envelope will have a minimum width passing through the center of the random matrix in the range from 2 mm to 100 mm.

A preferred metal shape memory filament is a nickel titanium wire having the diameter and length described above such wires may be obtained from a number of commercial sources, including Raychem Corporation, Menlo Park, California. The wires may then be formed into the preferred coil/random matrix geometry by conventional techniques. For example, the random matrix shape (as illustrated in Fig. 2 discussed below) may be permanently set into the wire by heating the wire while maintained in the desired configuration. To achieve the desired initial set, the wire should be heated to a temperature of about 500°C for a time in the range from about 5 minutes to 60 minutes. After cooling, the wire filament may then be wound and deformed plastically to the desired coil configuration. The coil configuration will be maintained at room temperature, with transformation back to the random matrix configuration being achieved by heating the coil to a temperature above about 20°C (the transition temperature will usually be in the range from 20°C to 70°C), whereby the coil will "recover" its initial random shape. Suitable shape memory plastic materials and methods for forming such materials into unexpanded and expanded configurations are described in U.S. Patent No. 4,950,258, the full disclosure of which has previously been incorporated herein by reference.

As most shape memory materials are not radiopaque, a separate radiopaque element or member will frequently be attached to the shape memory portion of the element described above. The radiopaque element or member may have any size or configuration which is readily apparent under fluoroscopic imaging and which is compatible with introduction and use of the embolic element. For example, in the case of the

un xpanded coil c nfiguration of the embolic element, the radiopaque member will conveniently be a separate ring member attached to at least one end of the coil, and typically being composed of platinum, gold, silver, tungsten, or other  
5 radiopaque material. Use of radiopaque ring is particularly compatible with introduction of the embolic element over delivery wire, as described in more detail hereinbelow.

For other modes of delivery, the radiopaque element or member can take other forms, for example, being mounted  
10 inside of the coil or elsewhere.

In many cases, it will be desirable to modify the embolic element in some way in order to enhance its thrombogenicity. For example, components composed of highly thrombogenic materials can be secured to the embolic element.  
15 Such components include threads, nets, foams, coatings, surface texturing, studs, projections, and any other structural feature that increases the thrombogenicity and/or surface area of the embolic element. Suitable thrombogenic materials include polyester, silk, ionomer (ethylene-vinyl  
20 copolymer), collagen, albumin, and the like. Particular examples include short silk or polyester threads tied at spaced-apart intervals along the length of the filament, a silk or polyester net disposed over the peripheral envelope defined by the expanded embolic element, an open cell foam  
25 within or over the matrix defined by the expanded embolic element, a collagen or other coating over the filament surface, and the like.

The embolic element may be delivered by any one of a variety of techniques employed for the delivery of known  
30 embolic coils, including those described in U.S. Patent Nos. 4,994,069; 5,108,407; 5,122,136; 5,217,484; 5,226,911; 5,234,437; 5,250,071; 5,261,916; and 5,312,415, the full disclosures of which are incorporated herein by reference. In some cases, it may be necessary to adapt or modify the  
35 construction of the embolic element to be compatible with the known delivery syst ms, for example, by including an anchor or a latch member at either or both ends of the embolic element to facilitate delivery.

A preferred delivery method and system according to the present invention employs a tubular guide catheter and a delivery wire, where the coil configuration of the embolic element may be pushed over the delivery wire through an axial lumen of the guide catheter to the target site. After release at the target site, the embolic element will be heated to or above the transition temperature in order to effect memory expansion to maximize the occlusive volume. In a particularly preferred aspect of the present invention, the delivery wire will have a helical section at its distal end. Typically, the helical section will include from 1 turn to 10 turns, preferably from 3 turns to 7 turns, with a diameter ( $d$  in Fig. 4) in the range from 2 mm to 20 mm, preferably 3 mm to 7 mm, and a width ( $w$  in Fig. 4) in the range from 1 mm to 20 mm, preferably to 3 mm to 7 mm. The helical section of the delivery wire will be disposed within the target site, typically within the target aneurysm, prior to advancement of the embolic element. The delivery wire will typically have an outside diameter in the range from about 0.25 mm to 1 mm, and a length in the range from about 60 cm to 300 cm. Typically, the distal-most 5 cm will be formed into the coil having the dimensions described above. As the embolic element is advanced over the helical section, it will assume a secondary helical or coiled configuration which matches that of the guidewire. The position of the embolic element can thus be confirmed within the target location prior to release. Moreover, inducing the secondary coiled configuration into the embolic element prior to release helps maximize the volume of the fully-extended element after heating.

After the releasing and heating of the embolic element, the delivery wire can be withdrawn back into the lumen of the guide catheter in order to disengage the expanded embolic element. The delivery catheter can be reinserted into the target location, however, in order to deliver a sufficient number of additional embolic elements in order to completely fill the target site. The guide catheter will be a small diameter tubular catheter having an axial lumen to permit introduction of the embolic element therethrough. Suitable

tubular catheters for use as guide catheters according to the present invention are described in copending Application Serial No. 08/151,320, filed on November 12, 1993, the full disclosure of which is incorporated herein by reference. The guide catheter will typically have a length in the range from about 50 cm to 200 cm and an internal lumen having a diameter in the range from about 0.3 mm to 3 mm.

The coil pusher will have a length in the range from about 50 cm to 300 cm, with a tracking portion formed over the distal-most 5 cm to 300 cm. The tracking portion will typically be a flexible tube, such as a polymeric tubular element, having a lumen size sufficient to be received over the delivery wire and a distal tip adapted to engage against a proximal end of the embolic coil. In the case of a coiled embolic element, the distal tip will typically be a flat face designed to engage against a flat proximal end of the coil. The proximal portion of the pusher may be a solid core pusher rod typically having a diameter in the range from about 0.2 mm to 1 mm. The delivery wire may be composed of a variety of material, including stainless steel, with the distal coil being formed from a radiopaque material, such as platinum.

The embolic element delivery system will further comprise a means for heating the embolic element during or after release of the element from the delivery wire. Conveniently, the heating means will comprise a lumen for directing a heated medium, such as heated saline or contrast medium, past the element to effect expansion, where the lumen may be provided by the central lumen of the tubular guide catheter. Systems for heated saline and other media under pressure for delivery to catheters are commercially available. Alternatively, the delivery system may incorporate other heating means, including but not limited to, electric resistance heaters, electric inductive heaters, laser radiation heaters, and the like.

Referring now to Figs. 1 and 2, the structure of an exemplary embodiment of an embolic element 10 constructed in accordance with the principles of the present invention will be described. Embolic element 10 is formed as a helical

coil 12 of a single wire filament composed of a shape memory alloy as discussed above. The coil includes a pair of radiopaque rings 14, one being disposed at each end of the coil. The rings may be attached to the coil using a  
5 conventional adhesive, such as an epoxy adhesive. The coil has a length of about 5 cm, an outside diameter of about 0.46 mm, and inside diameter of about 0.41 mm, where the wire filament has a diameter of about 0.025 mm and a length of about 150 cm. The embolic element 10 is shown in its  
10 unexpanded configuration in Fig. 1. After heating to above the transition temperature characteristic of the particular shape memory alloy selected, the wire filament of the coil will assume the random configuration illustrated in Fig. 2. The wire filament in its random configuration will define a  
15 peripheral envelope 16 shown in broken line in Fig. 2. The peripheral envelope generally defines the volume available for inducing thrombosis within the blood vessel after the element 10 has been deployed.

An exemplary guide catheter 20 for use in delivering  
20 the embolic element 10 is illustrated in Fig. 3. The guide catheter comprises a tubular body 22 which is optionally reinforced to enhance pushability and torqueability, as described in copending Application Serial No. 08/151,320, the full disclosure of which has previously been incorporated  
25 herein by reference. The guide catheter has a length of about 150 cm and an inside lumen diameter of about 0.5 mm.

Delivery wire 30 is illustrated in Fig. 4. The wire comprises a proximal wire body 32 having a length of about 170 cm and a diameter of about 0.25 mm. A distal helix 34 is  
30 formed at the distal end of the wire body 32 having a width w of about 5 mm and a diameter d of about 3 mm, and the coil will include about 4 full turns.

A suitable coil pusher 40 is illustrated in Fig. 5. Coil pusher 40 includes a proximal push rod 42 comprising a  
35 solid core stainless steel wire having a diameter of about 0.25 mm and a length of about 175 cm. A distal pusher section 44 has a length of about 35 cm and an inside diameter of about 0.3 mm. The coil pusher preferably includes a

radiopaque marker 46 near its distal tip. The pusher section 44 may be introduced over the delivery wire 30, as shown in broken line.

Referring now to Figs. 6-11, use of the delivery system of the present invention to deliver the exemplary embolic element 10 to an aneurysm A in a blood vessel BV will be described. Initially, guide catheter 20 is introduced through an opening AO to the aneurysm A over a conventional guidewire GW, as shown in Fig. 6. After the guide catheter 20 is in place, the guidewire GW is withdrawn and exchanged for the delivery wire 30, as illustrated in Fig. 7. After the coil section 34 of the delivery wire 30 is fully introduced into the interior of aneurysm A, the embolic element 10 may be introduced over the delivery wire. This is done by pushing the coil 10 with the pusher section 44 of the coil pusher 42, as illustrated in Fig. 8. The coil pusher 40 is advanced sufficiently so that the embolic element 10 is transferred entirely from the axial lumen of the guide catheter 20 and into the interior volume of the aneurysm A. Embolic element 10 will assume the helical configuration of the helical section 34 of the guidewire, as illustrated in Fig. 9. A heated medium may then be introduced through the axial lumen of the guide catheter in order to effect expansion of the embolic element 10 into its expanded, random configuration, as illustrated in Fig. 10. The delivery wire 30 may then be withdrawn so that the helical section 34 is removed from the interior of the embolic element 10, allowing the embolic element 10 to achieve its fully expanded, random configuration, as illustrated in Fig. 11.

It will be appreciated that a plurality of embolic elements 10 may be required to fill and initiate thrombosis of the entire internal volume of the aneurysm A. Additional embolic elements 10 may be introduced by repeating the steps just described a sufficient number of times in order to completely fill the internal volume.

In some cases, it will be desirable to provide a mechanism on the delivery catheter for selectively blocking premature or unintended release of the embolic element 10. An

exemplary delivery system 50 employing a gate 52 capable of such selective blockage is illustrated in Figs. 12-14. The gate 52 is disposed at the distal end of a delivery coil 54 which in turn is disposed at the distal end of delivery wire 56. A coil pusher 60 is also provided, generally as described above in connection with the earlier embodiments.

The gate 52 can have a variety of specific constructions, with the primary requirement being that it is selectively reconfigurable between a blocking, e.g., expanded, configuration and a non-blocking, e.g., non-expanded, configuration. The gate 52 could be actuated or deployed in a variety of ways, including mechanically, electrically, chemically, or the like. The preferred deployment, however, will be by exposure to a temperature above body temperature, typically by exposure to heated saline in a manner similar to heating of the embolic coil itself. Such heating could also be effected by electrically heating the gate, e.g., by introducing a low power electrical current therethrough. Other mechanical systems include use of a pull wire or other constraint to allow self-contraction of a gate element, chemical dissolution of a block which is present at the distal end of the catheter, or the like.

In the illustrated embodiment, the gate comprises a tube 70 having a plurality of axial slots 72 formed therein. The tube is composed of a heat memory alloy, such as Nitinol®, with the tube initially in its straightened, non-expanded configuration, as shown in Fig. 13. The tube is then heated and/or stressed into the expanded configuration of Fig. 12 in a manner so that the tube will remain in its expanded configuration until exposed to a temperature above body temperature, typically in the range from 20° C to 70° C, as set forth above for the embolic element. By employing both a gate 52 and embolic element 10 having substantially the same transition temperatures, it will be appreciated that the coil can be released and selectively transformed to its expanded configuration using the same delivery step for the heated saline. Note that the system 50 of Figs. 12-14 will also include an outer catheter sheath similar to the guide



catheter 20 illustrated in Fig. 3. Thus, the heated saline or other medium can be introduced through the lumen of the guid catheter (not shown).

5 As illustrated in Figs. 12-13, deployment of the embolic element 10 may be accomplished essentially as illustrated in Figs. 6-11, with the following difference: after the distal end of the delivery catheter is located at the desired target site, the heated medium will be introduced, causing both the contraction of the gate 52, as shown in  
10 Fig. 13, and the expansion of the embolic coil 10. The coil 10 can then be disengaged by advancing the coil pusher 60 in a forward direction, as illustrated in Fig. 14. Note, in Figs. 12-14, the delivery coil 54 is shown to have a relatively short length, only slightly longer than the embolic  
15 coil 10. The delivery coil 54, however, can readily be constructed to have a longer length, and also to have a coiled configuration, generally as shown and described regarding helix 34 of delivery wire 30 in Fig. 4.

20 Although the foregoing invention has been described in some detail by way of illustration and example, for purposes of clarity of understanding, it will be obvious that certain changes and modifications may be practiced within the scope of the appended claims.

**WHAT IS CLAIMED IS:**

- 1           1.    An embolic element comprising a filament  
2           composed of a shape memory material having a transition  
3           temperature, wherein the filament is in an unexpanded  
4           configuration at a first temperature at or below the  
5           transition temperature and assumes an expanded configuration  
6           when the temperature is raised to or above the transition  
7           temperature.
- 1           2.    An embolic element as in claim 1, wherein the  
2           unexpanded configuration is a coil.
- 1           3.    An embolic element as in claim 2, wherein the  
2           expanded configuration is a random matrix which defines a  
3           peripheral envelope which is larger in all dimensions than  
4           that of the unexpanded configuration.
- 1           4.    An embolic element as in claim 3, wherein the  
2           filament has a diameter in the range from 0.01 mm to 0.1 mm  
3           and a length in the range from about 30 cm to 1000 cm, wherein  
4           the unexpanded coil has a diameter in the range from 0.1 mm to  
5           1 mm and a length in the range from 2 mm to 600 mm, and  
6           wherein the peripheral envelope has a minimum dimension in the  
7           range from 2 mm to 100 mm.
- 1           5.    An embolic element as in claim 1, wherein the  
2           shape memory material is selected from the group consisting of  
3           a nickel titanium alloy having a transition temperature in the  
4           range from 20°C to 70°C and a plastic shape memory material.
- 1           6.    An embolic coil as in claim 1, further  
2           comprising a radiopaque segment attached to the wire filament.

1           7. An embolic coil as in claim 6, wherein the  
2 unexpanded configuration is a coil and wherein the radiopaque  
3 segment is a ring attached to at least one end of the coil,  
4 wherein the ring has a diameter which is substantially equal  
5 to that of the coil.

1           8. An embolic element as in claim 1, further  
2 comprising a thrombogenic component secured to the filament.

1           9. A system for selective occlusion of a target  
2 location within a blood vessel, said system comprising  
3 a catheter;  
4 an embolic element composed of a shape memory alloy  
5 having a transition temperature, an unexpanded configuration  
6 below the transition temperature sized to fit within or over  
7 the catheter, and an expanded configuration above the  
8 transition temperature which defines a peripheral envelope  
9 which is larger in all dimensions than that of the unexpanded  
10 configuration; and  
11 means on the catheter for heating the embolic  
12 element to the transition temperature when the element is  
13 positioned at the target location.

1           10. A system as in claim 9, wherein the catheter  
2 comprises a tubular body having an axial lumen which receives  
3 the embolic element in its unexpanded configuration  
4 therethrough.

1           11. A system as in claim 9, further comprising a  
2 delivery wire having a helical distal end, wherein the  
3 delivery wire may be positioned within the axial lumen of the  
4 catheter to provide an introducing path for the embolic  
5 element.

1           12. A system as in claim 11, wherein the unexpanded  
2 configuration of the embolic element is a coil, wherein the  
3 coil may be coaxially passed over the delivery wire and  
4 through the axial lumen of the catheter.

1           13. A system as in claim 12, wherein the coil is  
2       formed from a filament having a diameter in the range fr m  
3       0.01 mm to 0.1 mm and a length in the range from about 30 cm  
4       to 1000 cm, wherein the unexpanded coil has a diameter in the  
5       range from 0.1 mm to 1 mm and a length in the range from 2 mm  
6       to 600 mm, and wherein the peripheral envelope has a minimum  
7       dimension of in the range from 2 mm to 100 mm.

1           14. A system as in claim 13, wherein the coil on  
2       the delivery wire has a length in the range from 1 mm to  
3       20 mm, a diameter in the range from 2 mm to 20 mm, and  
4       consists of from 1 turn to 10 turns.

1           15. A system as in claim 12, wherein the delivery  
2       wire has a selectively deployable gate at its distal end.

1           16. A system as in claim 15, wherein the gate is  
2       deployable between an expanded configuration that blocks  
3       passage of the embolic coil over the distal end of the wire  
4       and a non-expanded configuration which permits passage.

1           17. A system as in claim 16, wherein the deployable  
2       gate is composed of a heat memory alloy that is in its  
3       expanded configuration at body temperature and which assumes  
4       its non-expanded configuration when exposed to a medium heated  
5       above body temperature.

1           18. A method for delivering an embolic element to a  
2       target site in a blood vessel, wherein said method comprises:  
3               positioning a delivery wire through a guide catheter  
4       so that a distal end of the delivery wire is disposed at the  
5       target site.  
6               introducing the embolic element over the delivery  
7       wire to the target site, wherein the embolic element is  
8       composed of a shape memory material and is in an unexpanded  
9       configuration which conforms to the delivery wire as the  
10      element is being introduc d; and

11                   expanding the embolic element by exposure to a  
12                   temperature above the transition temperature of the shape  
13                   memory alloy.

1                   19. A method as in claim 18, wherein the embolic  
2                   element is a filament having a coiled configuration prior to  
3                   expansion.

1                   20. A method as in claim 19, wherein expanding the  
2                   embolic element causes the filament to assume a random  
3                   configuration having a peripheral envelope which is larger in  
4                   all dimensions than that of the coiled configuration.

1                   21. A method as in claim 18, wherein the embolic  
2                   element is introduced over a helix formed at the distal end of  
3                   the delivery wire, wherein the embolic element assumes a  
4                   helical configuration defined by the delivery wire prior to  
5                   expansion.

1                   22. A method as in claim 18, wherein the embolic  
2                   element is expanded by flushing a heated liquid medium through  
3                   the guide catheter and past the embolic element at the target  
4                   site.

1                   23. A method as in claim 18, further comprising  
2                   selectively permitting release of the embolic element from the  
3                   delivery wire.

1                   24. A method as in claim 23, wherein the  
2                   selectively permitting step comprises exposing a heat memory  
3                   alloy gate to a temperature above body temperature, wherein  
4                   the gate reconfigures from an expanded configuration which  
5                   blocks passage of the element over the distal end of the  
6                   delivery wire to a non-expanded configuration which permits  
7                   passage of the element over the distal end of the delivery  
8                   wire.

1           25. A method for occluding a target location in a  
2 blood vessel, said method comprising  
3           introducing an embolic element composed of a shape  
4 memory alloy at the target location;  
5           heating the embolic element above a transition  
6 temperature to cause expansion of the element to an expanded  
7 configuration;  
8           wherein thrombus forms in the expanded embolic  
9 matrix to occlude at least a portion of the target location in  
10 the blood vessel.

1           26. A method as in claim 25, wherein the target  
2 location is an aneurysm.

1           27. A method as in claim 26, wherein the embolic  
2 element is introduced in an unexpanded coil configuration over  
3 a delivery wire.

1           28. A method as in claim 27, wherein the delivery  
2 wire has a helical distal tip disposed in the aneurysm,  
3 wherein the coiled embolic element assumes a helical  
4 configuration as it travels over the distal helix of the  
5 delivery wire.

1           29. A method as in claim 28, wherein the expanded  
2 configuration of the embolic element defines a peripheral  
3 envelope which is larger in all dimensions than that of the  
4 coiled configuration.

1           30. A method as in claim 25, wherein the embolic  
2 element is heated by flushing a heated liquid medium past the  
3 embolic element at the target site.

1           31. A method as in claim 27, further comprising  
2 selectively permitting release of the embolic element from the  
3 delivery wire.

1           32. A method as in claim 31, wherein the  
2 selectively permitting step comprises exposing a heat memory  
3 alloy gate to a temperature above body temperature, wherein  
4 the gate reconfigures from an expanded configuration which  
5 blocks passage of the element over the distal end of the  
6 delivery wire to a non-expanded configuration which permits  
7 passage of the element over the distal end of the delivery  
8 wire.

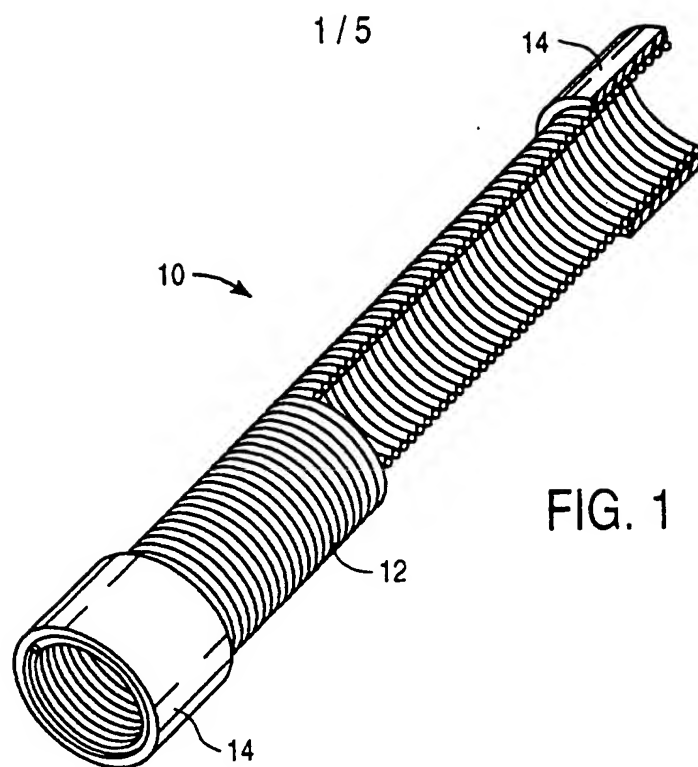


FIG. 1

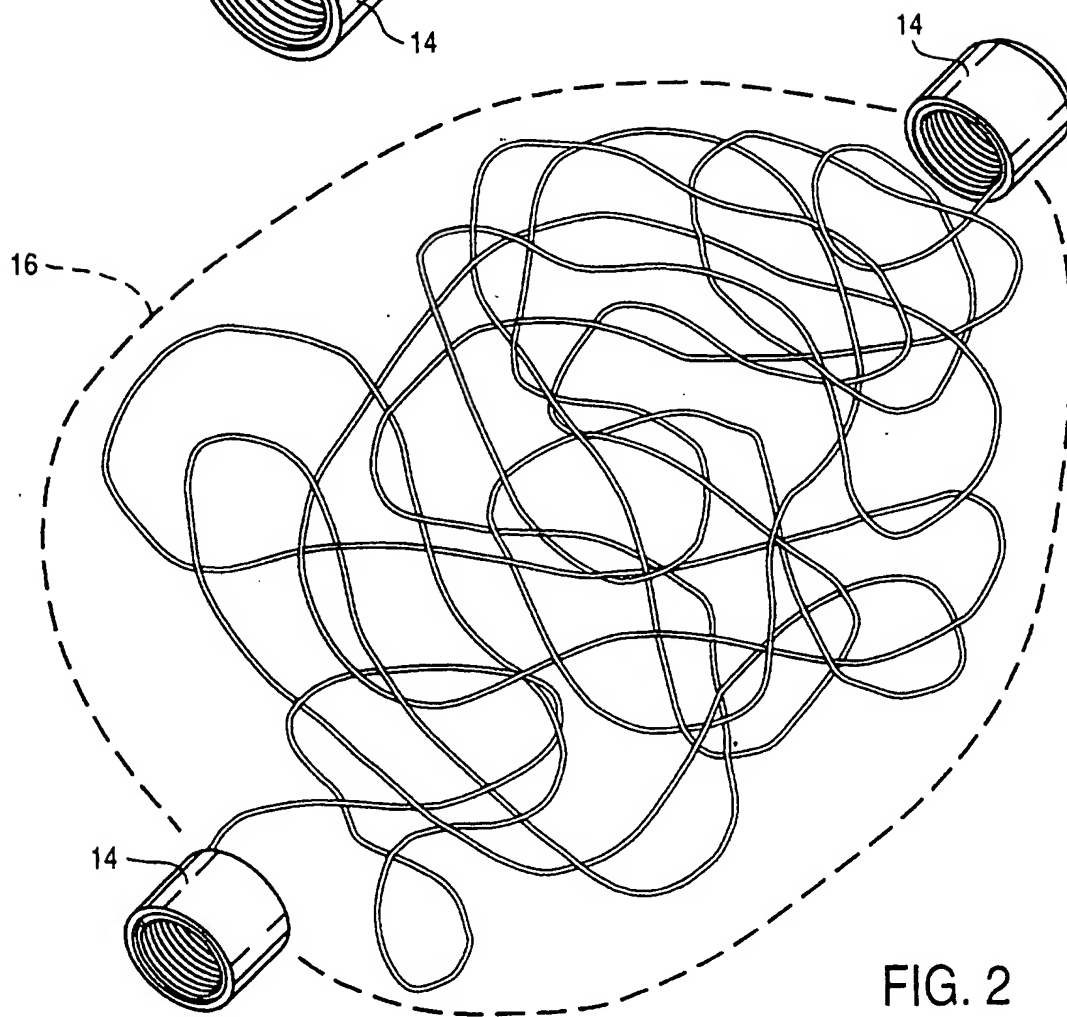


FIG. 2



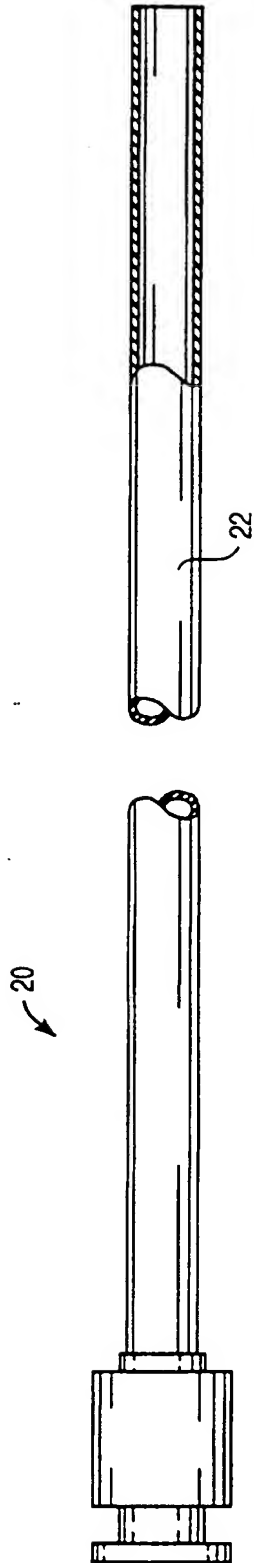


FIG. 3

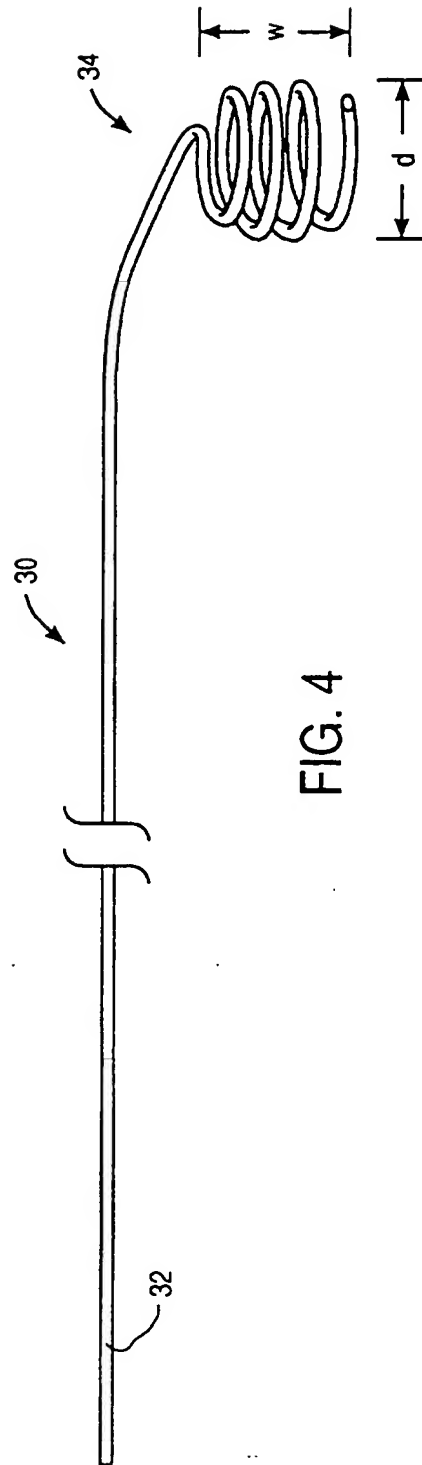


FIG. 4

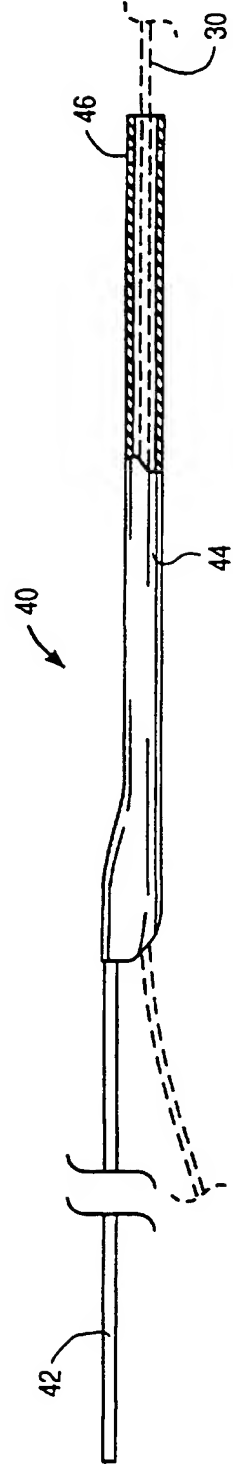


FIG. 5

3/5

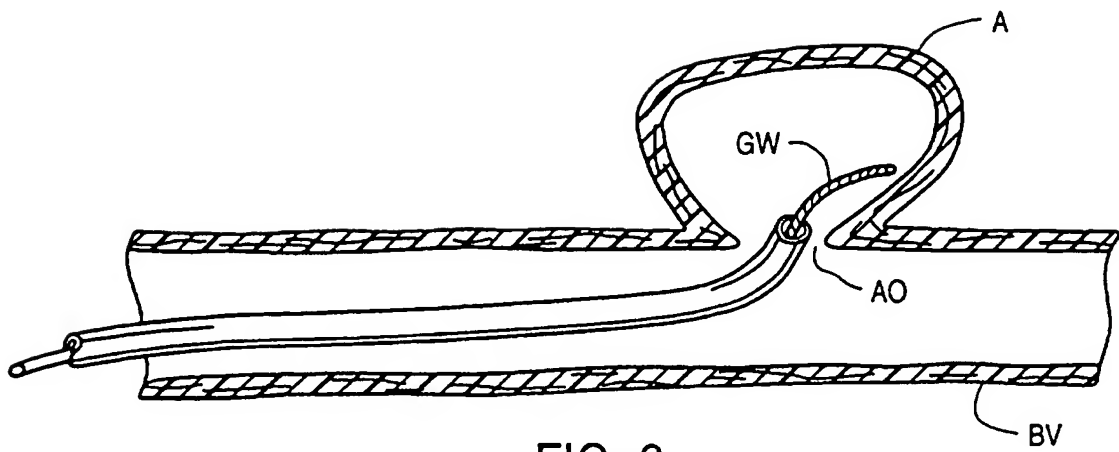


FIG. 6

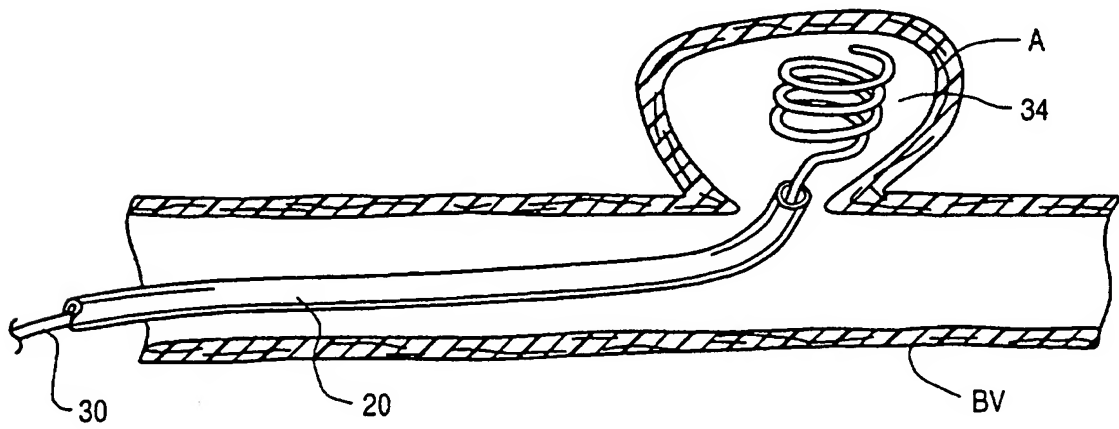


FIG. 7

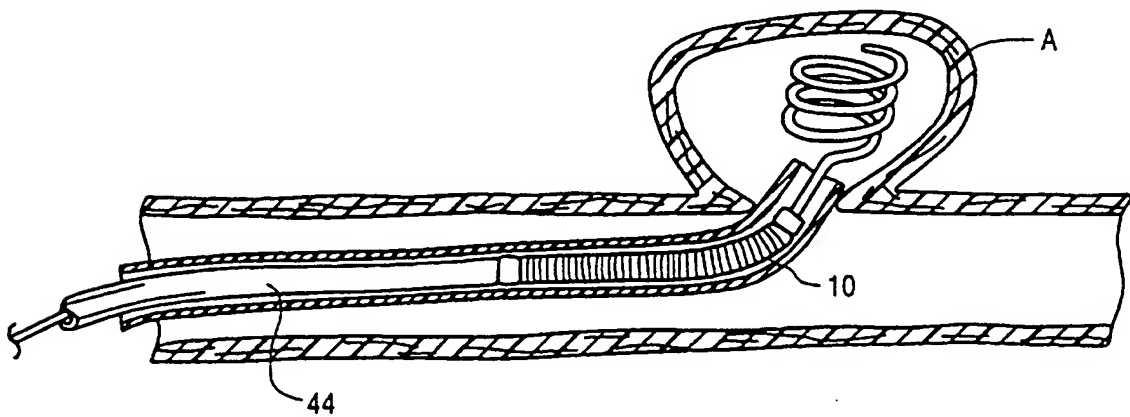


FIG. 8

4 / 5

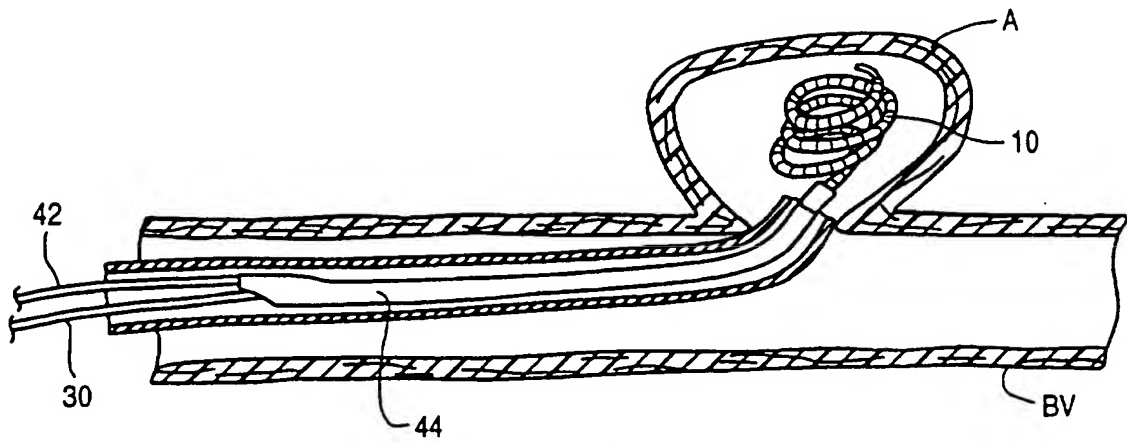


FIG. 9

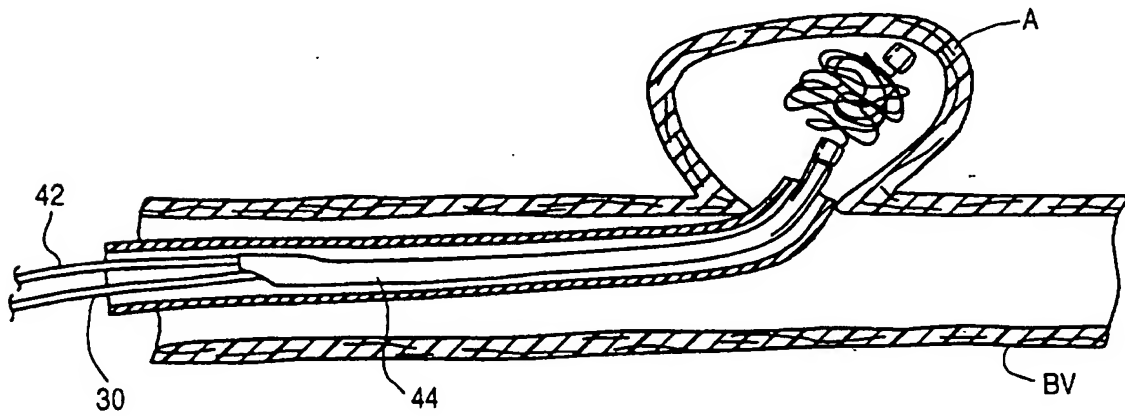


FIG. 10

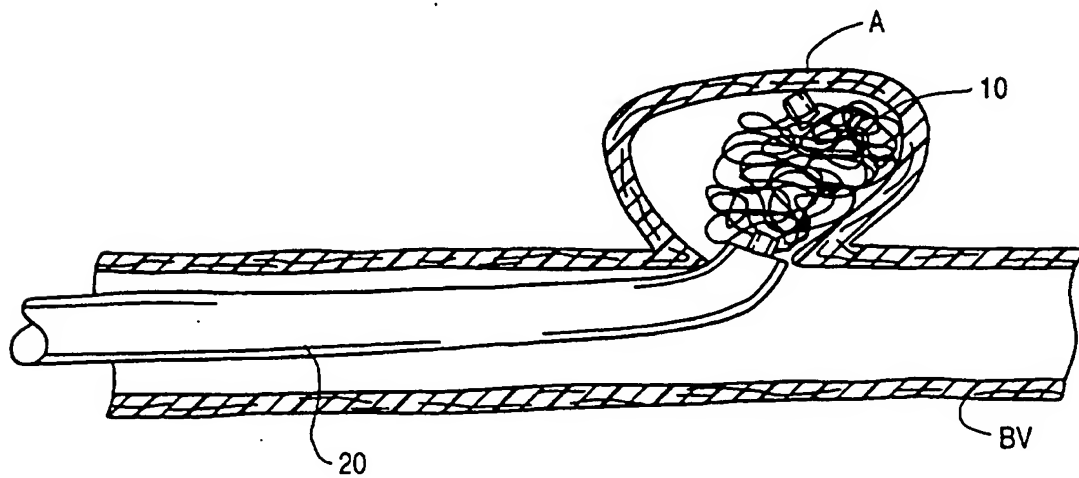


FIG. 11

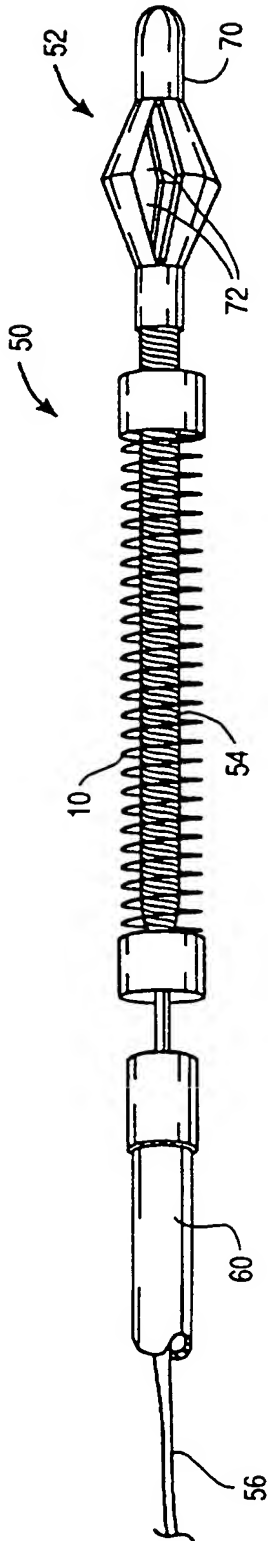


FIG. 12

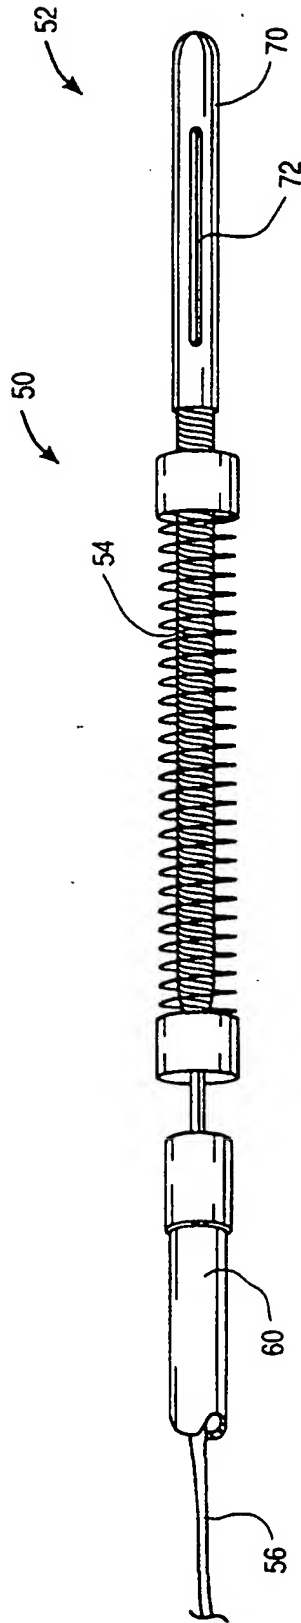


FIG. 13

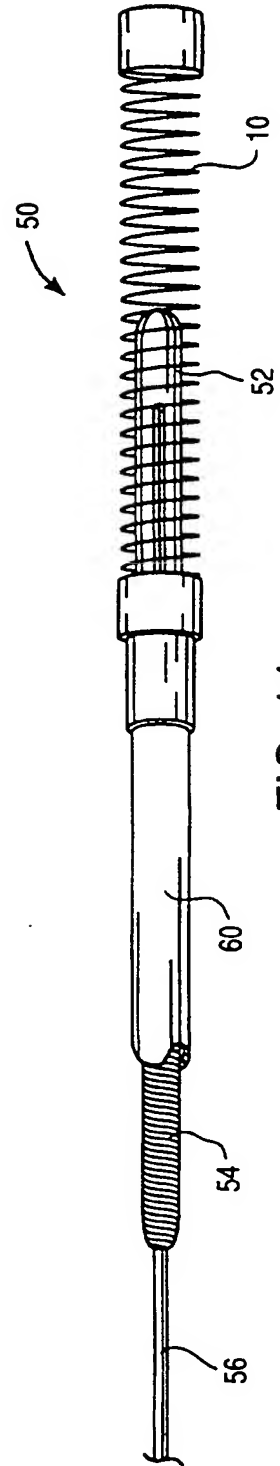


FIG. 14

## INTERNATIONAL SEARCH REPORT

 International application No.  
 PCT/US95/16022

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) : A61B 17/00

US CL : 606/200

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 128/772, 784, 898, 899; 606/1, 32, 41, 191, 194, 195, 198, 200; 623/1, 12

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US, A, 5,226,911 (CHEE ET AL.) 13 July 1993, see Fig. 2.	8
Y	US, A, 4,994,069 (RITCHART ET AL.) 19 February 1991, see entire document.	1-6, 8-10
Y	US, A, 4,503,569 (DOTTER) 12 March 1985, see entire document.	1-6, 8-10
Y	US, A, 5,312,415 (PALERMO) 17 May 1994, see column 4 lines 24-34.	6

☐ Further documents are listed in the continuation of Box C.
 ☐ See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be part of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"G" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

27 MARCH 1996

Date of mailing of the international search report

06 MAY 1996

 Name and mailing address of the ISA/US  
 Commissioner of Patents and Trademarks  
 Box PCT  
 Washington, D.C. 20231

Facsimile No. (703) 305-3230

Authorized officer

 FOR  
 WILLIAM LEWIS

Telephone No. (703) 308-0060